NEW ARRIVAL!

ACE PLUS Bracket

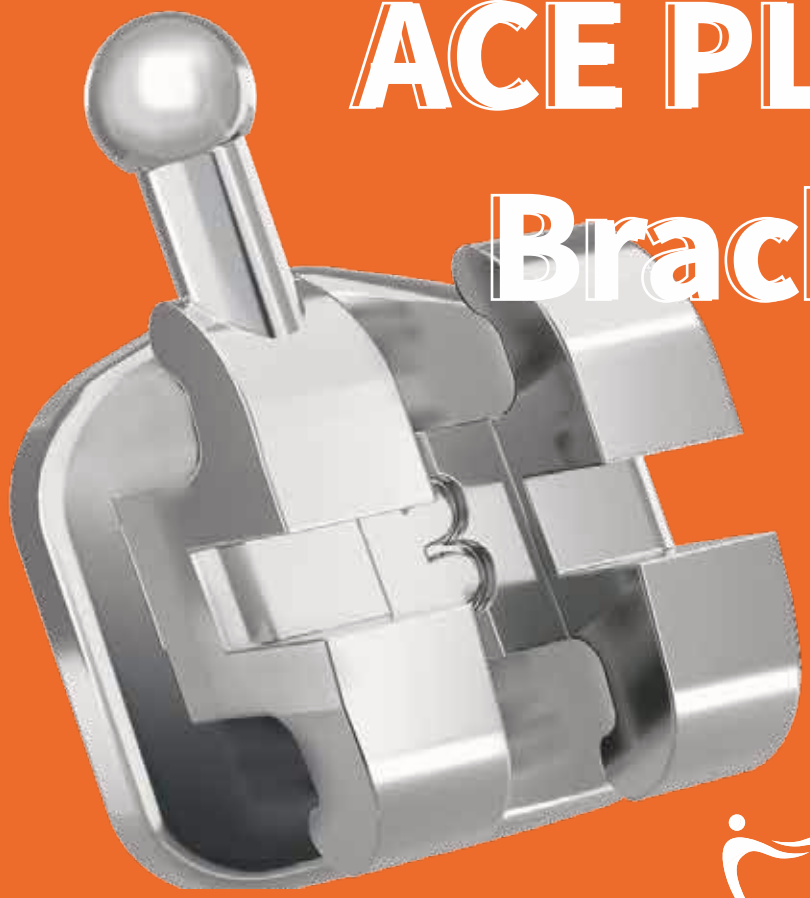

IMD®
INNOVATION FOR YOU

The bracket you have been waiting for.

Find us on Facebook and Instagram with IMDMEDICAL

Web: www.imdmedical.com

Toll Free: +86 400 8202 169

ACE PLUS Bracket

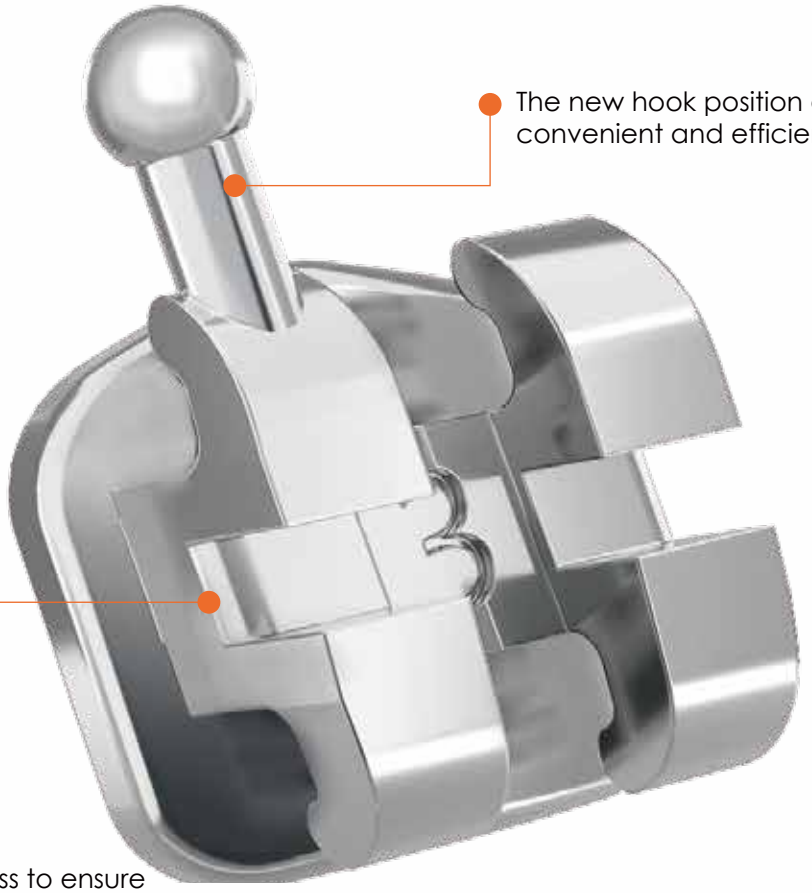

- The new hook position design is more convenient and efficient for traction.
- Special polishing process to ensure smooth slot for easier wire insertion
- Mini size for patient comfort
- Precision casting with 17-4PH sainless steel in wings and slot for strength and silky smooth.



An 80 gauge mesh forming a superior surface area of interlocking retention



Arch Base for increased bond strength and accurate bracket placement



Torque in face design for proper tooth positioning and level slot alignment

ACE PLUS Bracket

BRACKET I.D. CHART

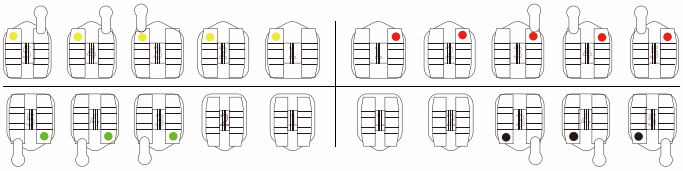



ACE PLUS series Roth* mini bracket kits

	.018 in.	.022 in.
U/L 5×5 Hook on 3、4 & 5	KIT18-212-00CBCHKW	KIT18-222-00CBCHKW

MAXILLARY

Roth*

Tooth	Torque	Angle	Offset	M/D in mm	R/L	Color Code	Hook	Item Number .018	Item Number .022
Central (U1)	+12°	+5°	0°	3.20	UR	●	-	18-212-11W	18-222-11W
					UL	●		18-212-21W	18-222-21W
Lateral (U2)	+8°	+9°	0°	2.75	UR	●	-	18-212-12W	18-222-12W
					UL	●		18-212-22W	18-222-22W
Cuspid (U3)	-2°	+10°	0°	3.00	UR	●	-	-	-
					UL	●			
					UR	●	D	18-212-13HKW	18-222-13HKW
					UL	●		18-212-23HKW	18-222-23HKW
Bicuspid (U4)	-7°	0°	0°	2.85	UR	●	-	-	-
					UL	●			
					UR	●	M	18-212-14HKW	18-222-14HKW
					UL	●		18-212-24HKW	18-222-24HKW
Bicuspid (U5)	-7°	0°	0°	2.85	UR	●	-	-	-
					UL	●			
					UR	●	M	18-212-15HKW	18-222-15HKW
					UL	●		18-212-25HKW	18-222-25HKW

MANDIBULAR

Tooth	Torque	Angle	Offset	M/D in mm	R/L	Color Code	Hook	Item Number .018	Item Number .022
Anteriors (L1)	-1°	0°	0°	2.40	LR		-	18-212-41W	18-222-41W
					LL			18-212-31W	18-222-31W
Anteriors (L2)	-1°	0°	0°	2.40	LR		-	18-212-42W	18-222-42W
					LL			18-212-32W	18-222-32W
Cuspid (L3)	-11°	+7°	0°	3.00	LR	●	-	-	-
					LL	●			
					LR	●	D	18-212-43HKW	18-222-43HKW
					LL	●		18-212-33HKW	18-222-33HKW
1st Bicuspid (L4)	-17°	0°	0°	2.85	LR	●	-	-	-
					LL	●			
					LR	●	D	18-212-44HKW	18-222-44HKW
					LL	●		18-212-34HKW	18-222-34HKW
2nd Bicuspid (L5)	-22°	0°	0°	2.85	LR	●	-	-	-
					LL	●			
					LR	●	D	18-212-45HKW	18-222-45HKW
					LL	●		18-212-35HKW	18-222-35HKW

* Our version of the Roth Rx is not implied to be an exact version of any other system, nor do we claim any endorsement of Dr. Roth. Our version of the McLaughlin, Bennett, and Trevisi system is not implied to be an exact version of any other system, nor do we claim any endorsement of doctors McLaughlin, Bennett, and Trevisi.

ACE PLUS Bracket

BRACKET I.D. CHART

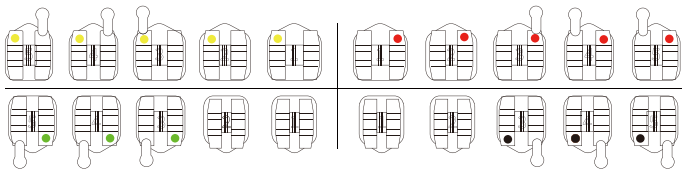



ACE PLUS series McBeTr* mini bracket kits

	.018 in.	.022 in.
U/L 5×5 Hook on 3、4 & 5	KIT18-312-00CBCHKW	KIT18-322-00CBCHKW

MAXILLARY — McBeTr*

Tooth	Torque	Angle	Offset	M/D in mm	R/L	Color Code	Hook	Item Number .018	Item Number .022
Central (U1)	+17°	+4°	0°	3.20	UR		-	18-312-11W	18-322-11W
					UL			18-312-21W	18-322-21W
Lateral (U2)	+10°	+8°	0°	2.75	UR		-	18-312-12W	18-322-12W
					UL			18-312-22W	18-322-22W
Cuspid (U3)	-7°	+8°	0°	3.00	UR		-	-	-
					UL				
					UR		D	18-312-13HKW	18-322-13HKW
					UL			18-312-23HKW	18-322-23HKW
Bicuspid (U4)	-7°	0°	0°	2.85	UR		-	-	-
					UL				
					UR		M	18-312-14HKW	18-322-14HKW
					UL			18-312-24HKW	18-322-24HKW
Bicuspid (U5)	-7°	0°	0°	2.85	UR		-	-	-
					UL				
					UR		M	18-312-15HKW	18-322-15HKW
					UL			18-312-25HKW	18-322-25HKW

MANDIBULAR

Tooth	Torque	Angle	Offset	M/D in mm	R/L	Color Code	Hook	Item Number .018	Item Number .022
Anteriors (L1)	-6°	0°	0°	2.40	LR		-	18-312-41W	18-322-41W
					LL			18-312-31W	18-322-31W
Anteriors (L2)	-6°	0°	0°	2.40	LR		-	18-312-42W	18-322-42W
					LL			18-312-32W	18-322-32W
Cuspid (L3)	-6°	+3°	0°	3.00	LR		-	-	-
					LL				
					LR		D	18-312-43HKW	18-322-43HKW
					LL			18-312-33HKW	18-322-33HKW
1st Bicuspid (L4)	-12°	+2°	0°	2.85	LR		-	-	-
					LL				
					LR		D	18-312-44HKW	18-322-44HKW
					LL			18-312-34HKW	18-322-34HKW
2nd Bicuspid (L5)	-17°	+2°	0°	2.85	LR		-	-	-
					LL				
					LR		D	18-312-45HKW	18-322-45HKW
					LL			18-312-35HKW	18-322-35HKW

* Our version of the Roth Rx is not implied to be an exact version of any other system, nor do we claim any endorsement of Dr. Roth. Our version of the McLaughlin, Bennett, and Trevisi system is not implied to be an exact version of any other system, nor do we claim any endorsement of doctors McLaughlin, Bennett, and Trevisi.

IMD®
INNOVATION FOR YOU

INNOVATIVE MATERIAL AND DEVICES, INC.
Add: Building#5, NO. 615 Fengdeng Rd., Jiading District,
Shanghai 201801, China.
Web: www.imdmedical.com